

Product Name: SGA Calibration Standard 3

Part Number: 1404006

Batch Number: C3SGA008


Method of Analysis: Spectrophotometric titration

DataSet Numbers: 05K-0207

pK_a values:

Equation	Measured value	Specification value
$X + H = XH$	9.211	9.2 ± 0.2
$XH + H = XH_2$	5.046	5.0 ± 0.2

UV profile:

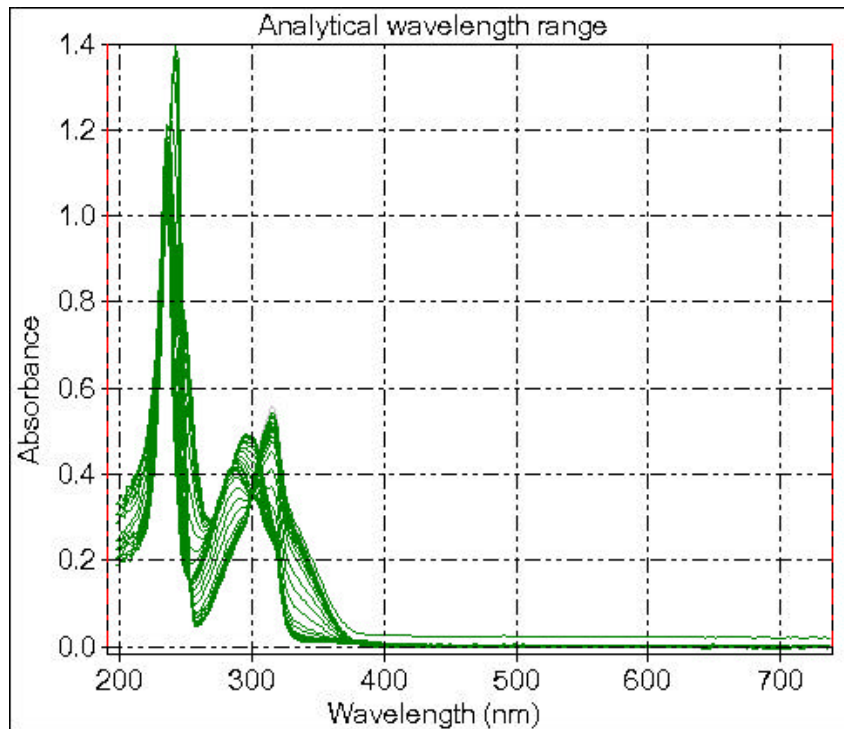

This product has been tested by the Quality Control Laboratory of Sirius Analytical Instruments Limited and conforms to the specifications described above.

Approved:.....

Carolyn Hibbert

.....
Carolyn Hibbert, Quality Assurance Co-ordinator

Certificate Date:..... 03 November 2005

C3SGA008.doc